

FIG. 1

FIG. 2 is a perspective view of the device 100, showing the foot 104 positioned within the device 100.

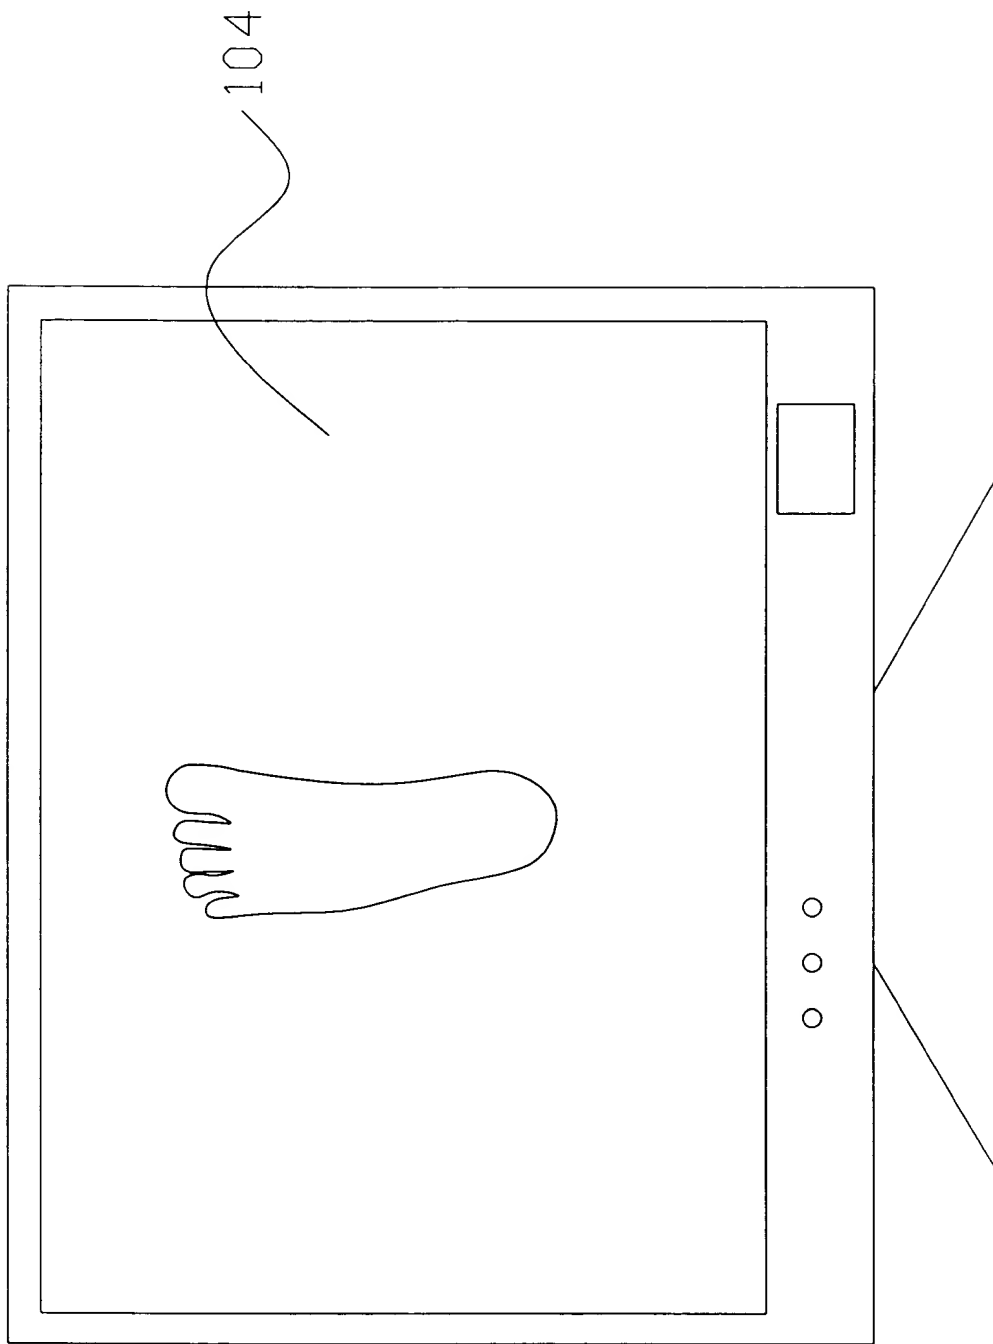


FIG. 2

100

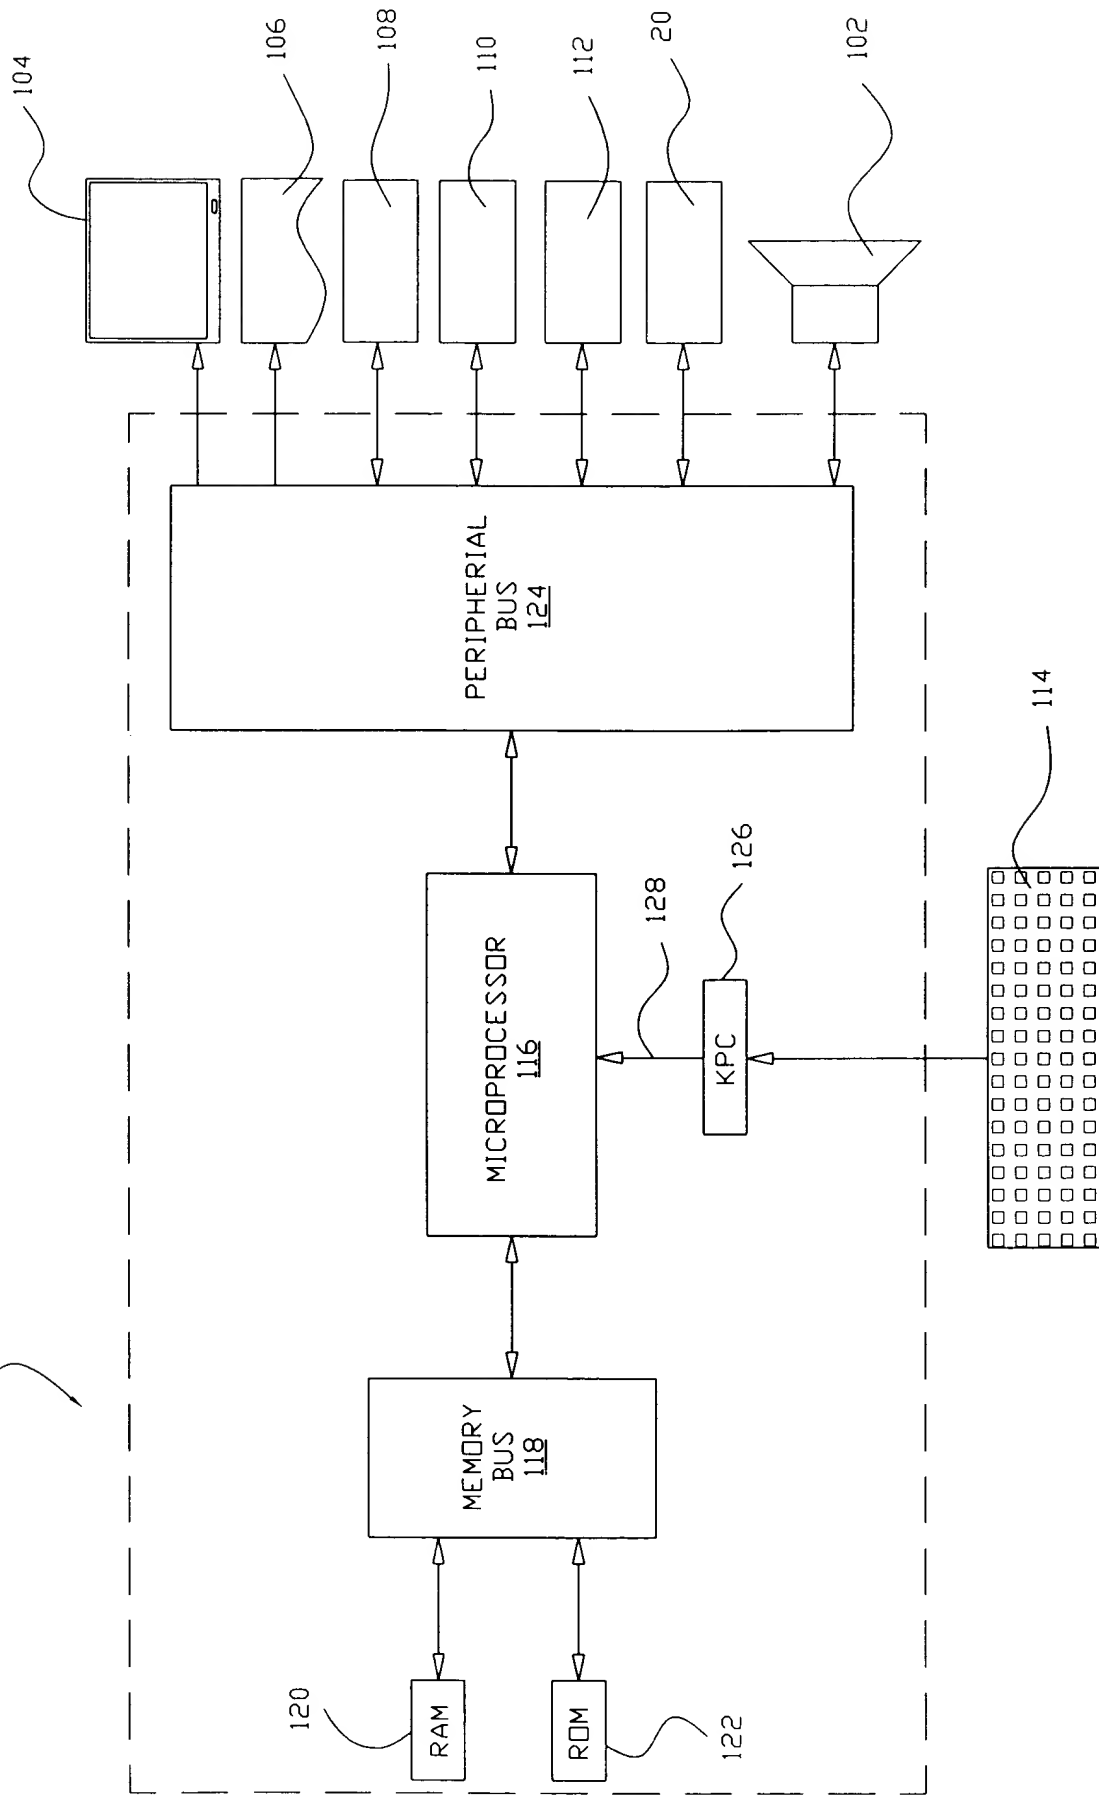


FIG. 3

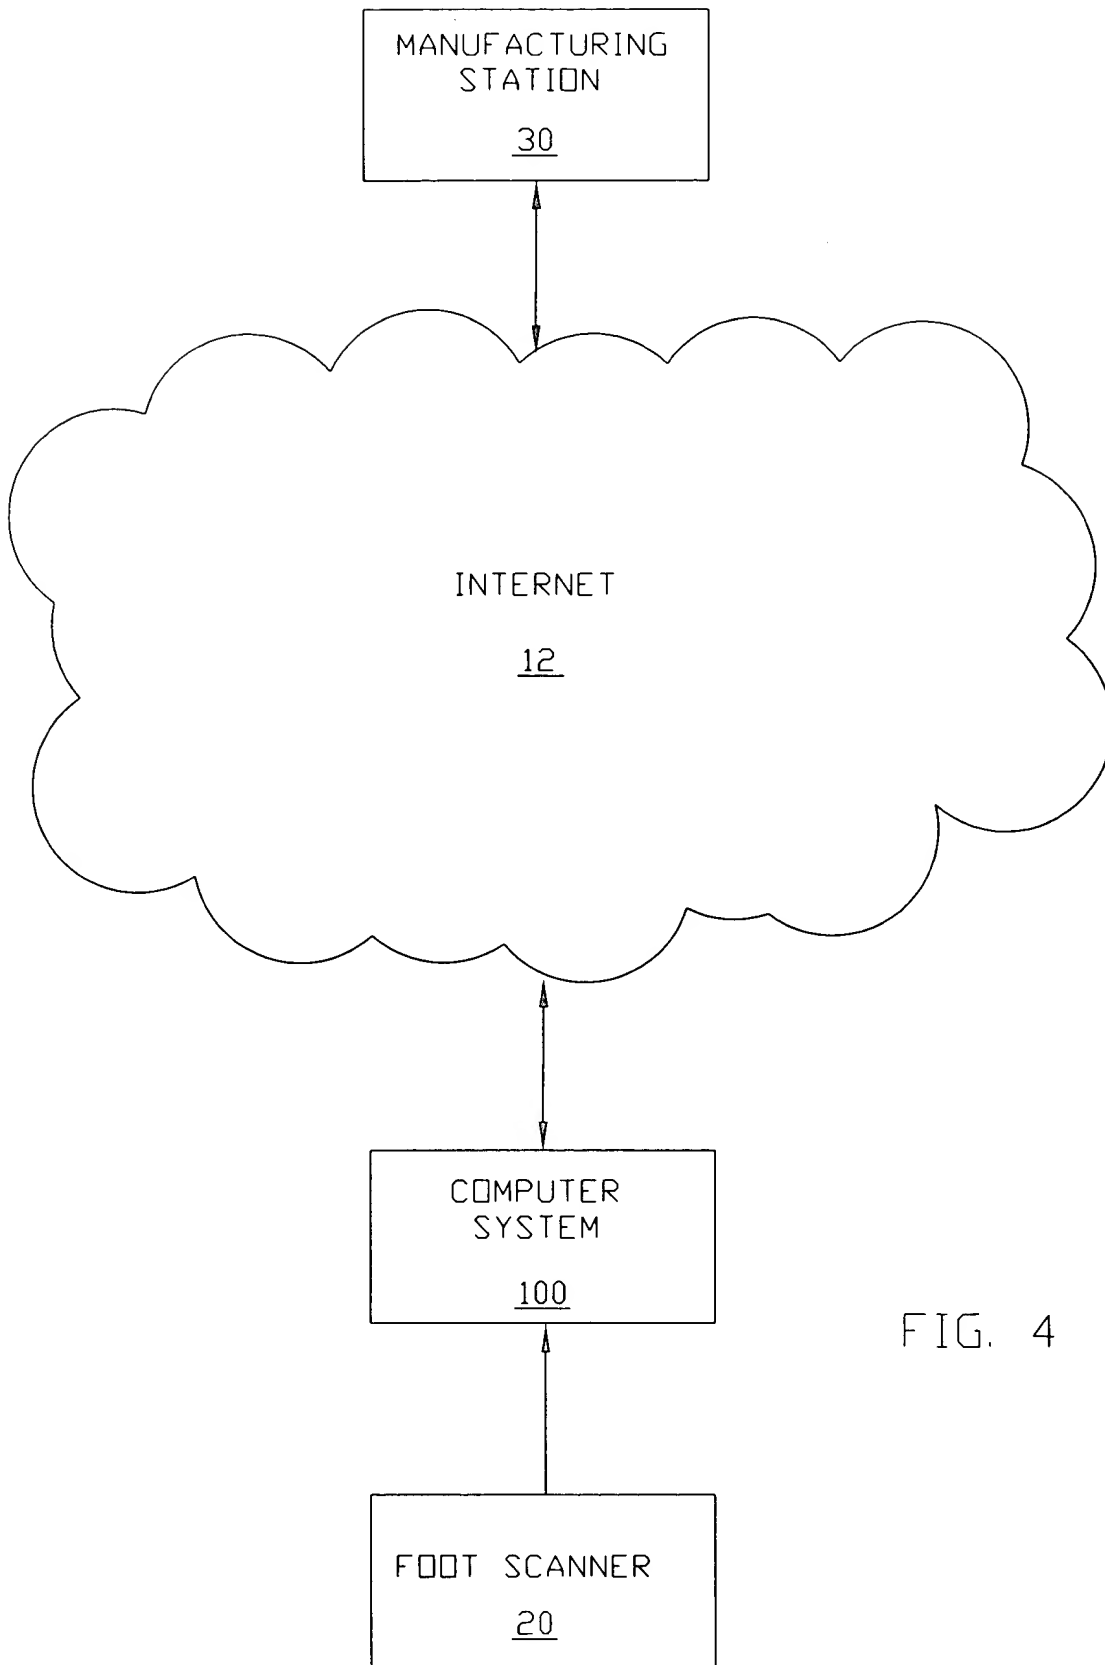


FIG. 4

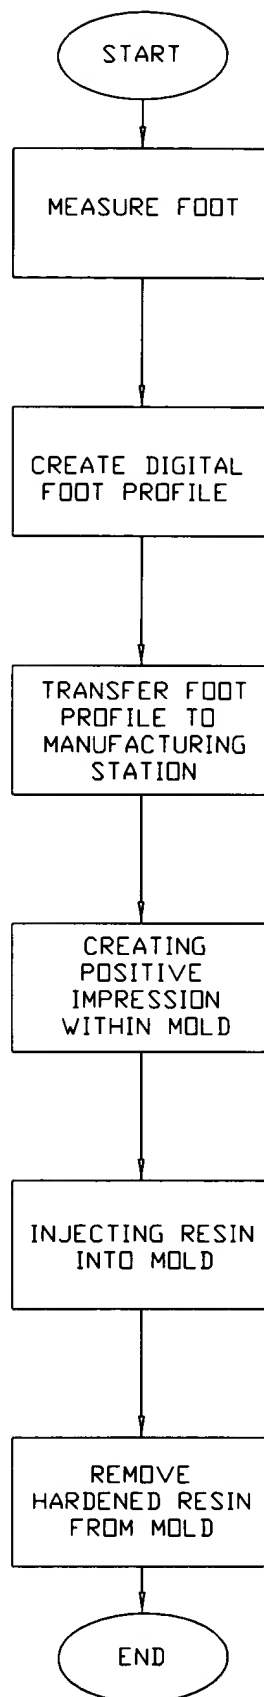


FIG. 5



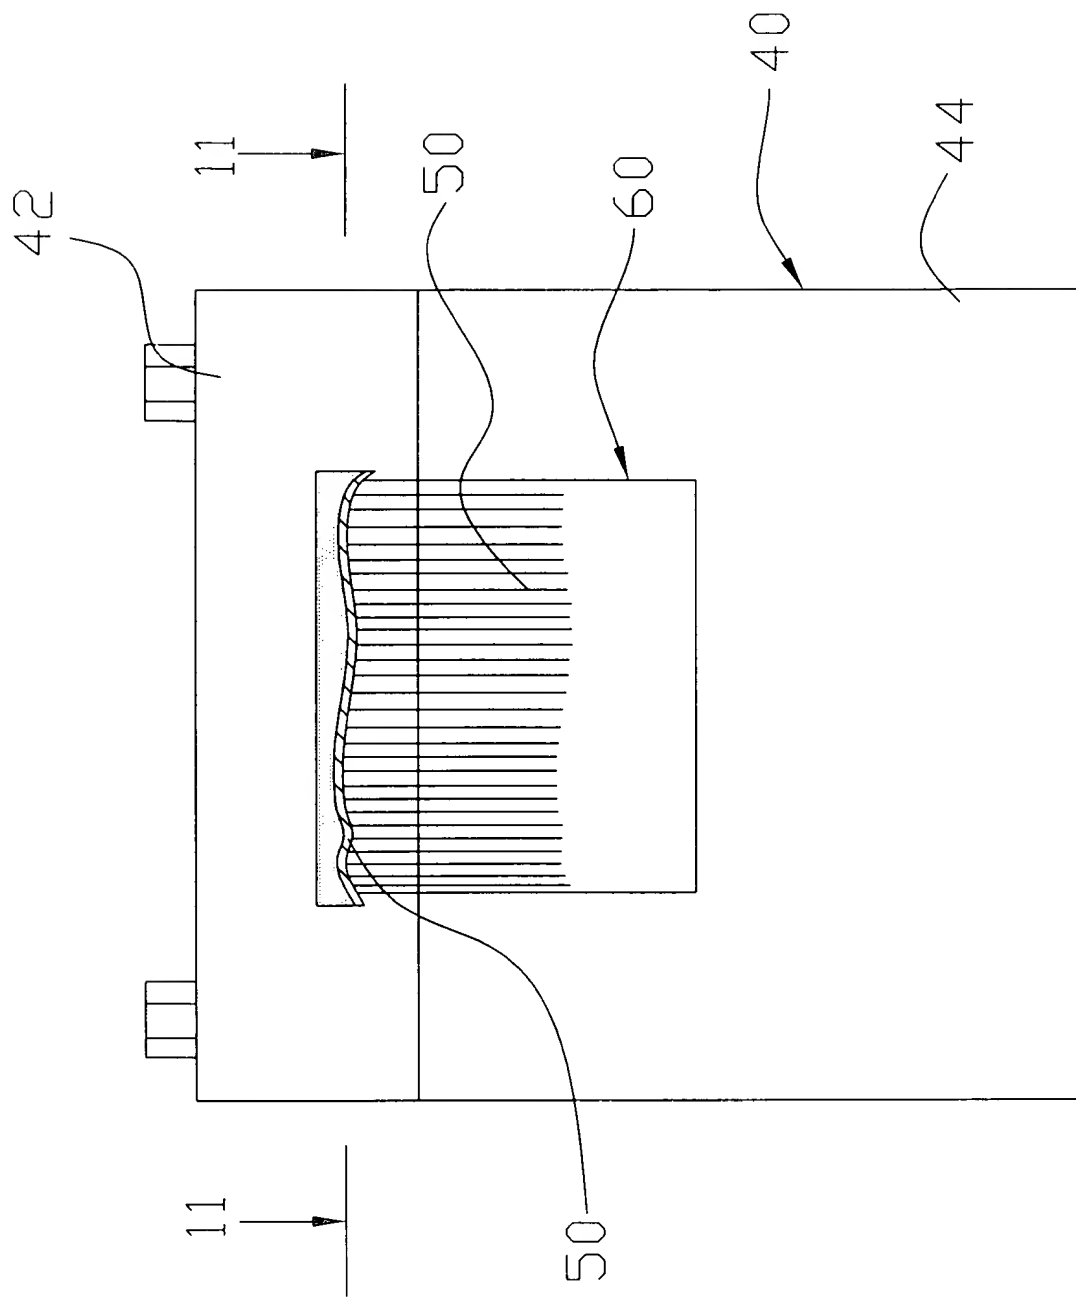


FIG. 7

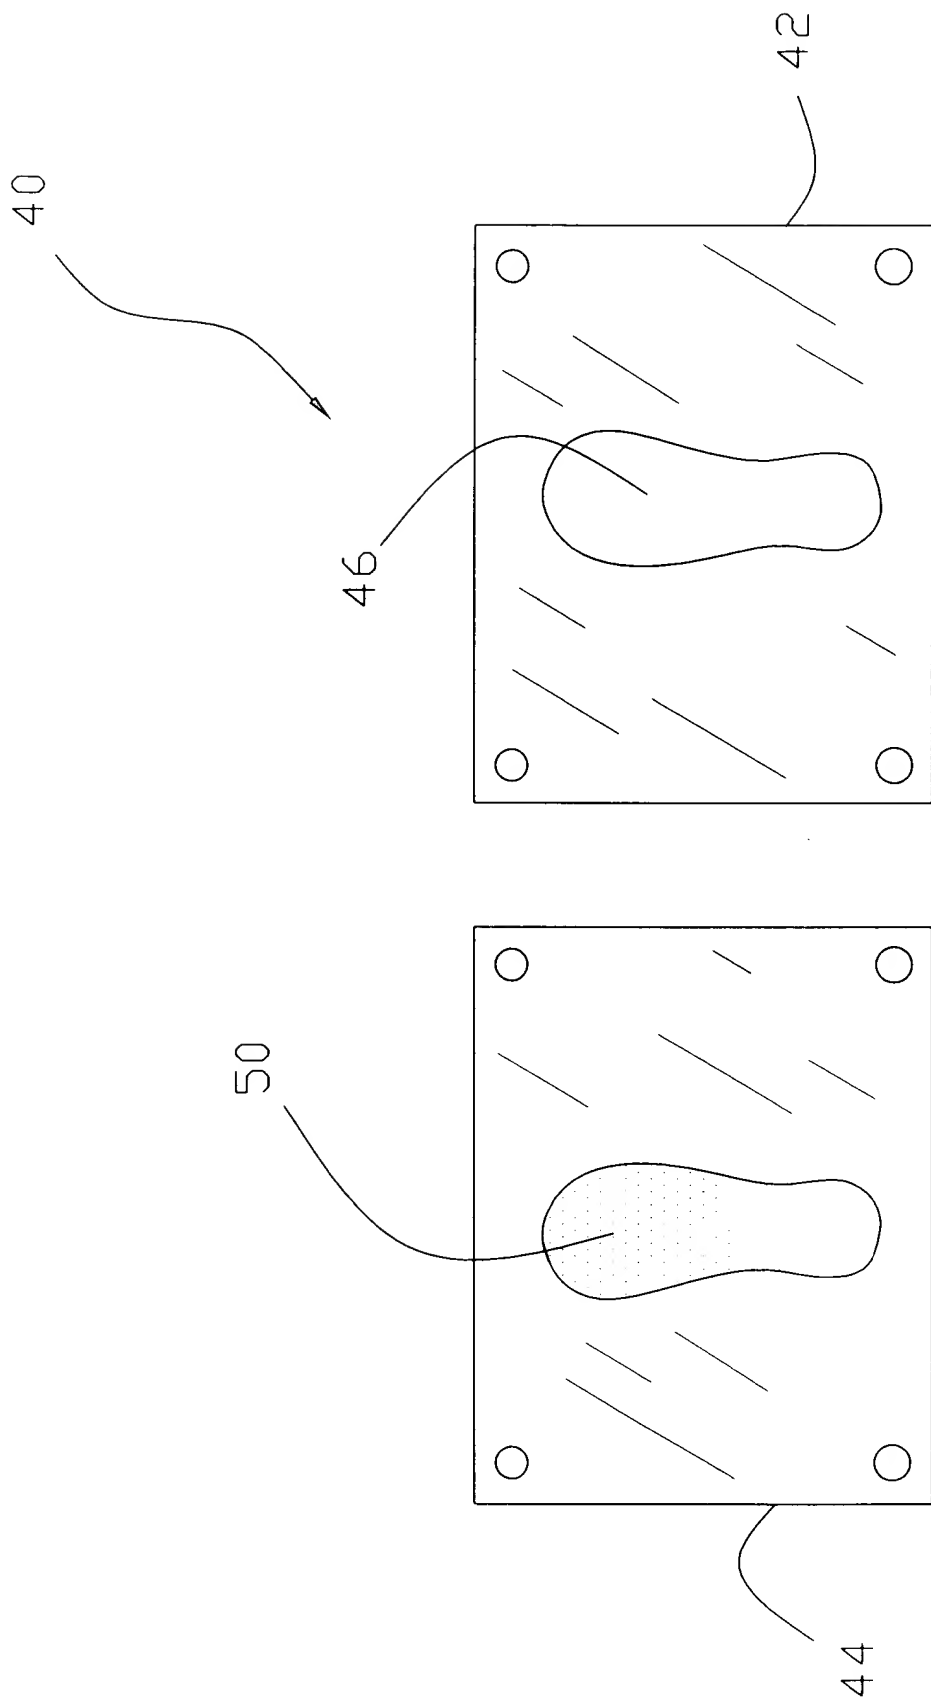


FIG. 8



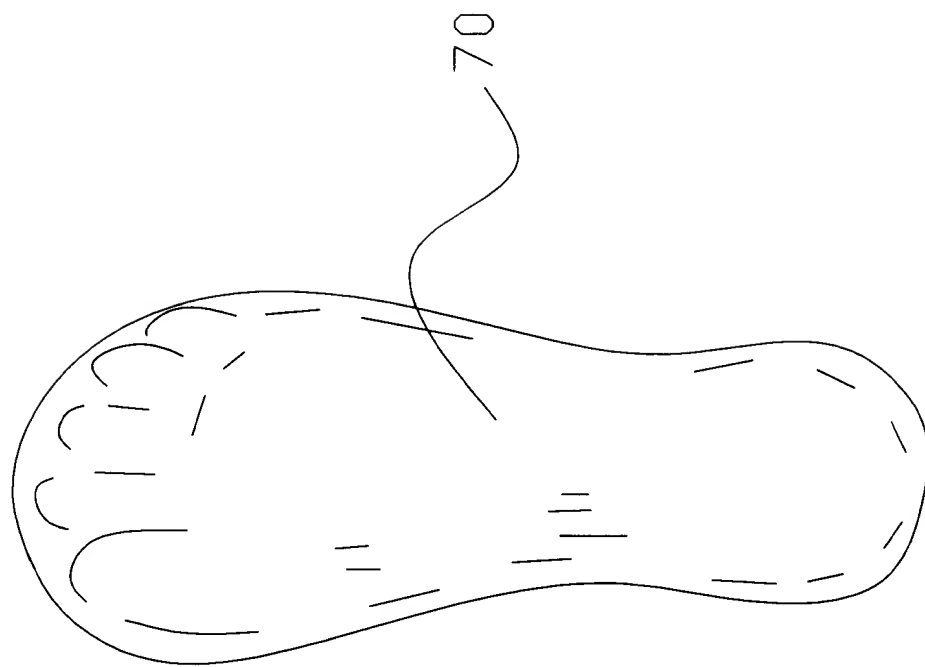


FIG. 9

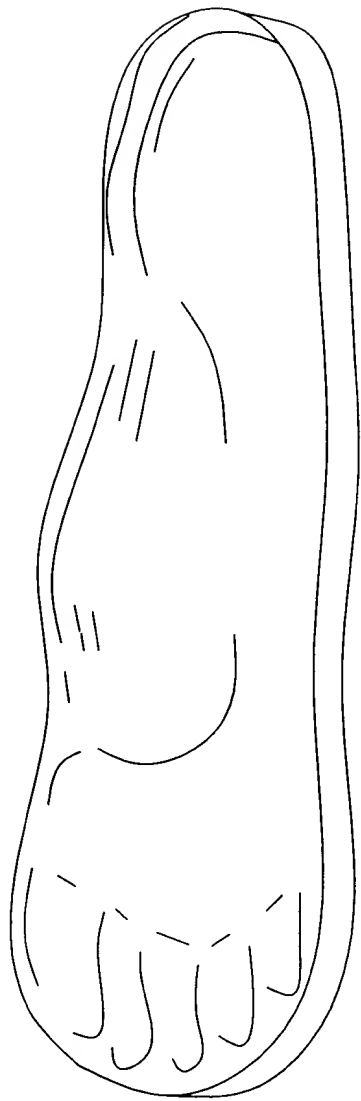


FIG.10

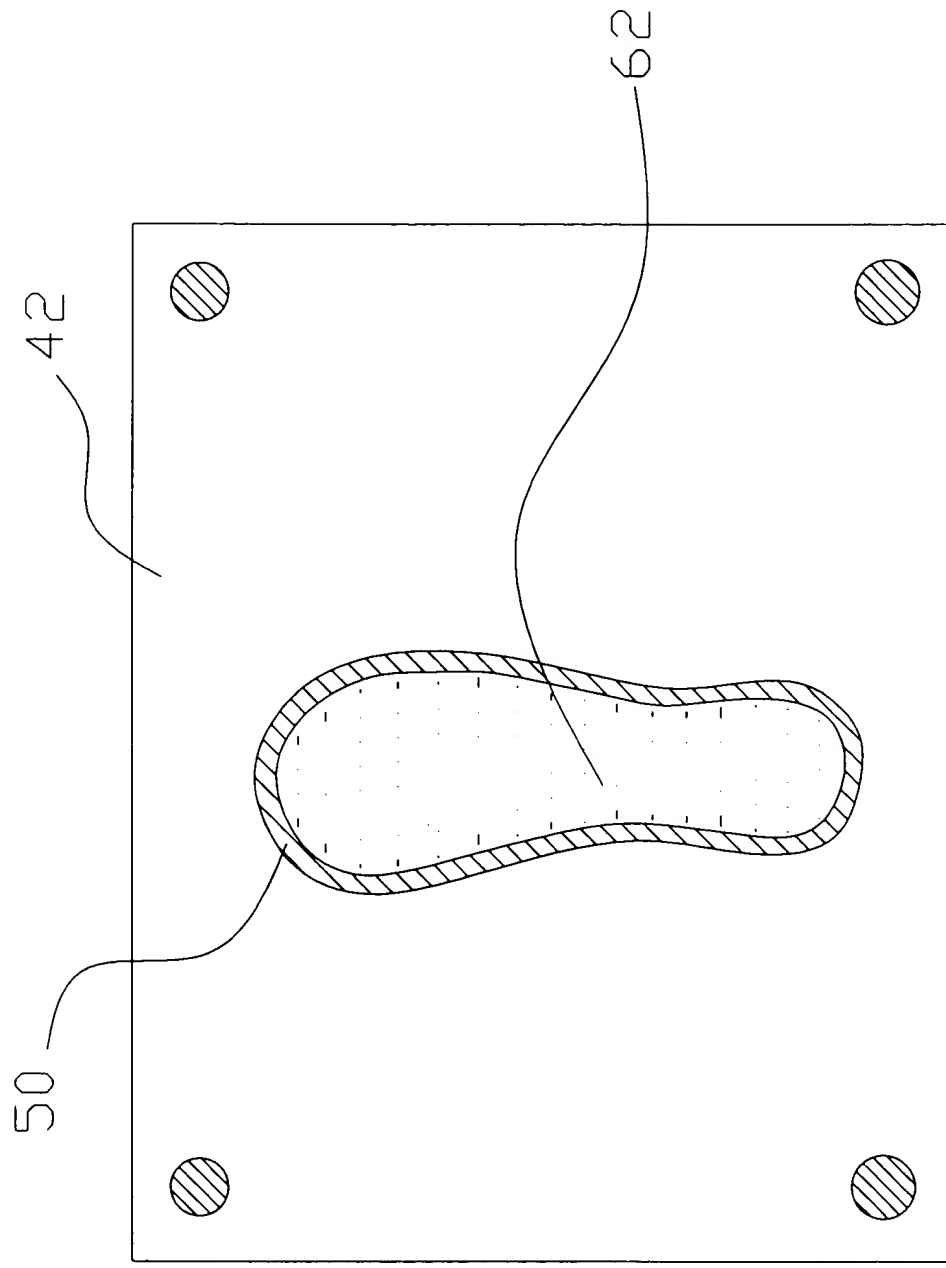


FIG. 11